



BioPoly® RS Patella System

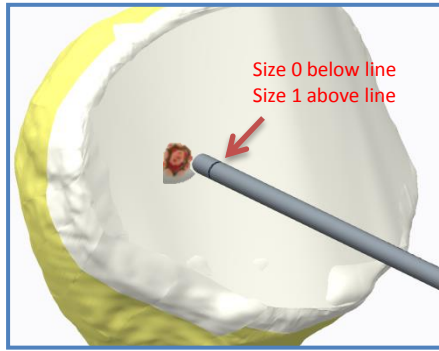


Assess defect depth

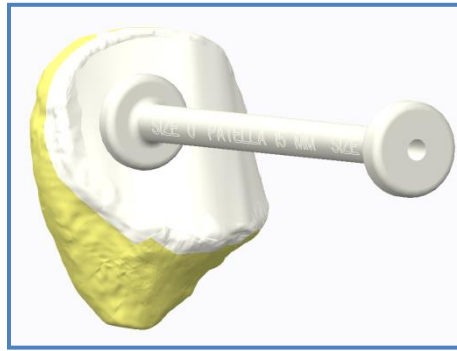


Assess defect size




Place drill guide & insert pilot nail

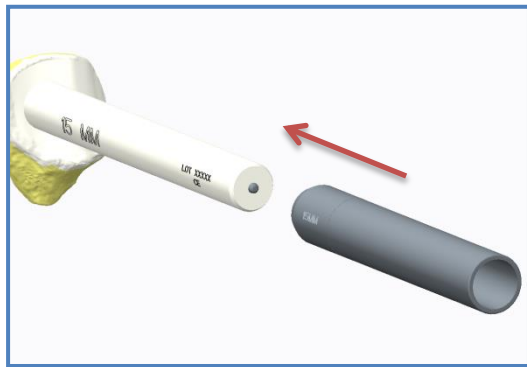


Place guide tube & cut cartilage

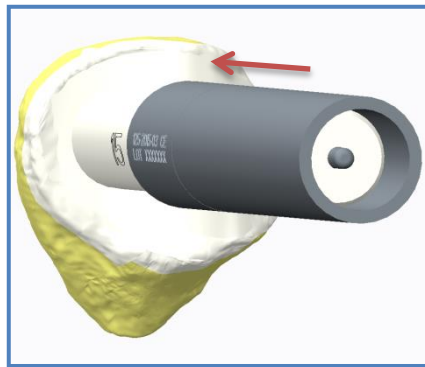


Place reaming cannula

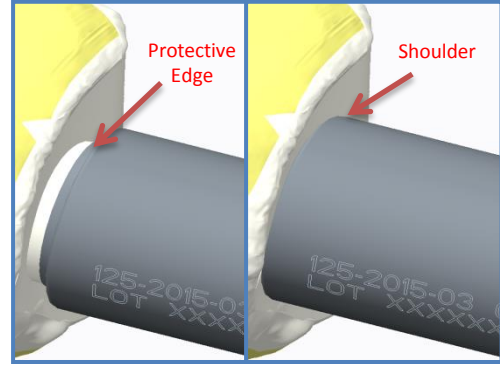


Ensure shoulder resting on cartilage

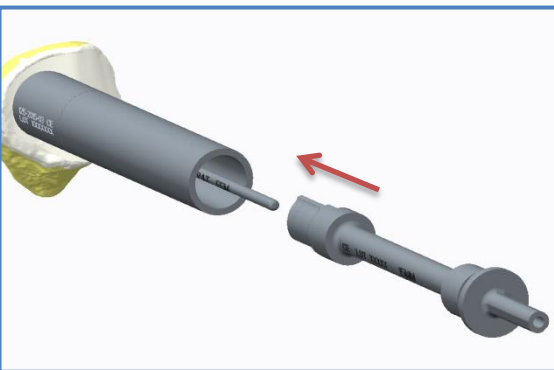


Ream

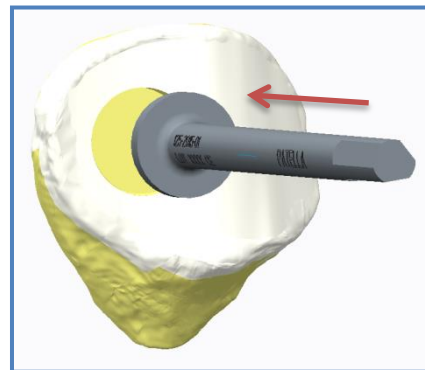


Drill stem hole

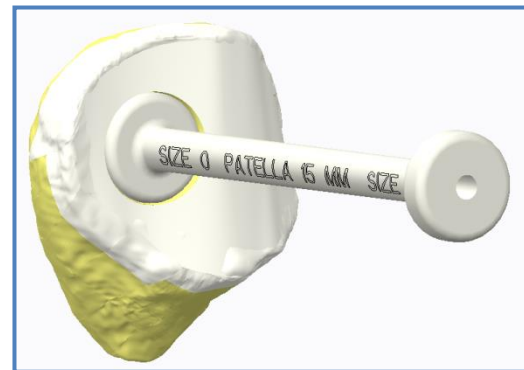


Trial

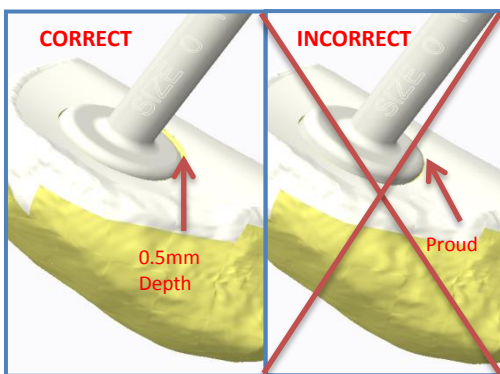

Assess

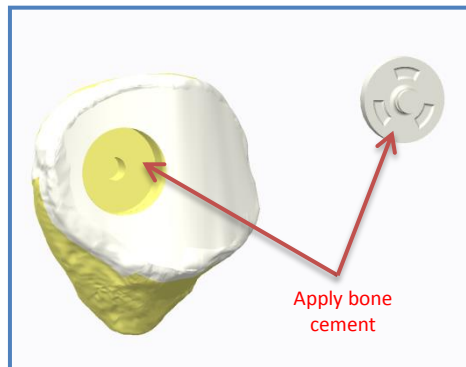

Apply bone cement
push into place

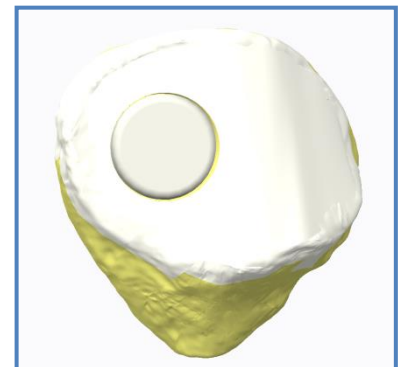

Implant properly placed